

अति आवश्यक / महत्वपूर्ण / द्वारा फैक्स

# उत्तर प्रदेश पुलिस तकनीकी सेवायें मुख्यालय,

चतुर्थ तल, जवाहर भवन, अशोक मार्ग, लखनऊ-226001

पत्रांक-टीएस / एमओडी-120 / 2015-16 (एफएसएल)

दिनांक, नवम्बर 27, 2015

सेवा में

निदेशक,  
सूचना एवं जन सम्पर्क विभाग, (विज्ञापन प्रभाग),  
उत्तर प्रदेश, लखनऊ।

विषय- आधुनिकीकरण योजना के अन्तर्गत निम्नलिखित उपकरणों के कयार्थ निविदा आमंत्रित किया जाना।

महोदय,

कृपया उपर्युक्त विषयक विज्ञापन की 05 प्रतियाँ अंग्रेजी / हिन्दी में मय सी0डी0 के संलग्न कर इस अनुरोध के साथ प्रेषित की जा रही है कि उक्त नोटिस को व्यापक प्रचार-प्रसार वाले प्रमुख दैनिक समाचार पत्र हिन्दी / अंग्रेजी जैसे दिल्ली / लखनऊ / मुम्बई से प्रकाशित होने वाले दैनिक जागरण, अमर उजाला, दि प्वाइनियर, टाइम्स आफ इन्डिया तथा द न्यू इन्डियन एक्सप्रेस आदि प्रमुख समाचार पत्रों में प्रकाशित करने का कष्ट करें।

2/ इस सम्बन्ध में निविदा के विज्ञापन की स्वच्छ टंकित प्रति एवं एमएस वर्ड (फारमेट में सी0डी0) साफ्ट कापी भी वेब साइट पर प्रसारित कराने हेतु संलग्न की जा रही है।

3/ अनुरोध है कि कृपया संलग्न निविदा को प्राथमिकता के आधार पर प्रकाशित कराने का कष्ट करें।

संलग्नक-विज्ञापन की प्रति 05 प्रतियों में।

2-सी0डी0की साफ्ट कापी।

भवदीय

(संजय कुमार)

अपर पुलिस अधीक्षक, तकनीकी सेवायें,  
निमित्त-पुलिस महानिरीक्षक, तकनीकी सेवायें,  
लखनऊ।

प्रतिलिपि-पुलिस महानिरीक्षक, प्रो0 / बजट, उ0प्र0 पुलिस मुख्यालय, इलाहाबाद को सूचनार्थ एवं आवश्यक कार्यवाही हेतु प्रेषित है।

2-प्रतिलिपि- पुलिस अधीक्षक / सहायक निदेशक, उ0प्र0 पुलिस कम्प्यूटर केन्द्र, लखनऊ को विज्ञापित निविदा की एक प्रति एवं सी0डी0 संलग्न कर इस आशय से प्रेषित है कि उक्त निविदा को उ0प्र0 पुलिस की वेबसाइट पर भी प्रसारित कराने का कष्ट करें। संलग्नक-यथोपरि

3-प्रतिलिपि-निदेशक, एफएसएल, लखनऊ लखनऊ को सूचनार्थ एवं व्यापक प्रचार-प्रसार एवं आवश्क कार्यवाही हेतु।

4-प्रतिलिपि- नोटिस बोर्ड तकनीकी सेवायें, लखनऊ को चस्पा करने हेतु।

# उत्तर प्रदेश पुलिस तकनीकी सेवायें मुख्यालय,

चतुर्थ तल, जवाहर भवन, अशोक मार्ग, लखनऊ

संख्या-टीएस-एमओडी-120 / 2015-16(एफएसएल)

दिनांक -नवम्बर, 27 2015

## निविदा सूचना

- 1- उत्तर प्रदेश पुलिस हेतु निम्न उपकरणों की सील बन्द निविदा भारतीय मैनुफैक्चरर/डीलर/रजिस्टर्ड फर्म /विदेशी मैनुफैक्चरर के अधिकृत विक्रेता से आमंत्रित की जाती है।
- 2- निविदा प्रपत्र व उपकरण से सम्बन्धित तकनीकी स्पेशीफिकेशन उत्तर प्रदेश पुलिस की वेबसाइट <http://uppolice.gov.in> से डाउनलोड किया जा सकता है। निविदा शुल्क के रूप में ₹0 300.00 का बैंक ड्राफ्ट/बैंकर चेक/एफडीआर पुलिस अधीक्षक/सहायक निदेशक, उ0प्र0पुलिस कम्प्यूटर केन्द्र लखनऊ के नाम देय होगा, जमा की जायेगी।
- 3- निविदा शुल्क किसी भी दशा में वापस नहीं किया जायेगा तथा निविदा स्वीकृत न होने की दशा में ईएमडी वापस कर दी जायेगी।
- 4- तकनीकी सेवायें मुख्यालय से नगद भुगतान पर टेण्डर डाकुमेंट्स विक्रय नहीं किये जायेंगे।
- 5- प्रत्येक टेण्डरकर्ता द्वारा टेण्डर की ईएमडीए डीडी/ एफडीआर / बैंक गारन्टी के रूप में, जो पुलिस अधीक्षक/सहायक निदेशक, उ0प्र0पुलिस कम्प्यूटर केन्द्र लखनऊ के नाम देय होगा, जमा की जायेगी।
- 6- सफल टेण्डरकर्ता द्वारा कयादेश मूल्य का 10 प्रतिशत धनराशि सिक्योरिटी मनी के रूप में जमा किया जायेगा, जो उपकरण के सन्तोषजनक ढंग से कार्य करने के उपरान्त उनके वारन्टी अवधि के उपरान्त वापस कर दी जायेगी।
- 7- तकनीकी स्पेशीफिकेशन के अनुसार प्रोप्राइटरी आइटम या उनके समतुल्य उत्पाद/सेवा अन्तराष्ट्रीय स्तर के स्वीकार होंगे। प्रोप्राइटरी उत्पाद या इसके समतुल्य उत्पाद/सेवा सम्बन्धित तकनीकी समिति का निर्णय अन्तिम निर्णय होगा।
- 8- उपकरणों की संख्या विभाग की आवश्यकतानुसार बढ़ायी जा सकती है तथा विभाग द्वारा बढ़ायी गयी संख्या को फर्म को निर्धारित अवधि में आपूर्ति करना होगा।
- 9- कम्पेरीजन माइक्रोस्कोप विद कम्प्यूटर इन्टरफेस उपकरण के तकनीकी स्पेशीफिकेशन में यदि कोई संशोधन होता है तो संशोधित तकनीकी स्पेशीफिकेशन दिनांक 10.12.2015 के पूर्व अपलोड किया जायेगा जिसे उत्तर प्रदेश पुलिस की वेबसाइट <http://uppolice.gov.in> से डाउनलोड किया जा सकता है।
- 10- समस्त टैक्स सहित न्यूनतम निविदा एल-1 पर विचारा किया जायेगा।
- 11- तकनीकी मुख्यालय द्वारा जनहित में किसी भी समय बिना कारण दर्शाये टेण्डर को निरस्त किया जा सकता है।

टेण्डर संख्या	आइटम	सं०	ईएमडी ( ₹0 में )	टेण्डर डाकुमेंट का मूल्य ( ₹0 में )
1. टीएस-मोड-94 / 2015-16 (एफएसएल)	डेस्कटॉप कम्प्यूटराइज्ड (माइयलर माडल)	01	22,000-00	200-00
2. टीएस-मोड-109 / 2015-16 (एफएसएल)	कम्पेरीजन माइक्रोस्कोप विद कम्प्यूटर इन्टरफेस	02	2,80,000-00	300 / -
3. टीएस-मोड-111 / 2015-16 (एफएसएल)	लैब कुलिंग डिवाइस(एयर कन्डीशनिंग)	02	2,00,000-00	300 / -
4. टीएस-मोड-135 / 2015-16 (एफएसएल)	लैब वर्क स्टेशन	08	2,0,000-00	200 / -

निविदा विक्री की तिथि

02.12.2015 समय 11.00 बजे पूर्वान्ह

निविदा फार्म विक्री करने की अन्तिम तिथि

16.12.2015 समय 11.00 बजे पूर्वान्ह

निविदा जमा करने की अन्तिम तिथि

16.12.2015 समय 02.00 बजे अपरान्ह

तकनीकी भाव पत्र खोले जाने की तिथि

16.12.2015 समय 04.00 बजे अपरान्ह

तकनीकी भाव पत्र पर कय समिति की बैठक

18.12.2015 समय 11.30 बजे पूर्वान्ह

वित्तीय भाव पत्र खोले जाने की तिथि

21.12.2015 समय 11.30 बजे पूर्वान्ह

वित्तीय भाव पत्र पर कय समिति की बैठक

21.12.2015 समय 04.00 बजे अपरान्ह

(संजय कुमार)

अपर पुलिस अधीक्षक, तकनीकी सेवायें,  
निमित्त-पुलिस महानिरीक्षक, तकनीकी सेवायें,  
लखनऊ।



**U. P. POLICE TECHNICAL SERVICES HEADQUARTERS**  
 IVth FLOOR JAWAHAR BHAWAN, ASHOK MARG, LUCKNOW-226 001  
 TENDER NO.: TS-MOD-120//2015-16(FSL)

DATED : November. 2) 2015

**NOTICE INVITING TENDER**

- 1- Sealed Tenders are invited from the Indian Manufacturers/registered firms/ Authorised agent of foreign manufacturer for purchase of the following equipment for the use of U.P. Police.
- 2- The tender form and tender document for item mentioned below along with Technical specification for Item given may be downloaded from U.P. Police website <http://uppolice.gov.in> on payment of Rs. 300-00 as fee of Tender cost documents in the form of DD/Banker Cheque/FDR/ in favour of of S.P.AD. Uttar Pradesh Police Computer Centre, payable at Lucknow.
- 3- Cost of tender document is not refundable, while earnest money(EMD) is refundable after tender process.
- 4- Tender documents will not be given on cash through Technical Head Quarter.
- 5- Each Tenderer will have to deposit an E.M.D. as mentioned against tender in the form of DD/ Banker's Cheque/FDR. in favour of S.P./AD. Uttar Pradesh Police Computer Centre, payable at Lucknow.
- 6- Successful tenderers will have to deposit a security money @ 10% of the order value, which will be returnable after expiry of warranty period.
- 7- For any specification which amounts to proprietary items its equivalent Product / Services of international quality will also be acceptable. However the decision of Technical Committee regarding Product / Services of International Quality will be final.
- 8 The Number of equipments may be increased as per need and the increased quantity will also have to be supplied within time stipulated by the Department.
- 9- The lowest bid will be decided on the basis of total cost (inclusive of all taxes.)
- 10- In condition of amendment in specification of item no.2 it will be uploaded before 10-12-2015.
- 11- The Technical Head Quarters may cancel the tender at anytime without assigning any reason for the same in the public interest.

Tender No.	Item	Qty	EMD (in Rs.)	Cost of Tender Document (in Rs.)
(I)TS-MOD-94/2015-16(FSL)	Desktop Computerised Moduler Model)	01	22,000-00	200-00
(II)TS-MOD-109/2015-16(FSL)	Comparison Microscope With Computer Interface	02	2,80,000-00	300-00
(III)TS-MOD-111/2015-16 (FSL)	Lab Cooling Device For Forfensic Lab(Air Conditioning)	02	2,00,000-00	300-00
(IV)TS-MOD-135/2015-1 (FSL)	Lab Work Station	08	40,000-00	200-00

Start of Sale of Tender documents from  
 Last date of sale tender documents  
 last date of deposit of tenders  
 Date of opening of Technical Bid  
 Date of Purchase committee meeting for technical evaluation  
 Date of opening of financial offer  
 Date of purchase committee meeting for financial evaluation

02-12-2015 at 11-00 am  
 16-12-2015 upto 11-00am  
 16-12-2015 upto 02-00pm  
 16-12-2015 at 04-00pm  
 18-12-2015 at 11-30am  
 21-12-2015 at 11-30am  
 21-12-2015 at 04-00 pm

(SANJAY KUMAR)

Addl. Supdt. of Police, Technical Services,  
 For- Inspector Genl. Of Police, Technical Services,  
 Lucknow.



TS-mod-94/2015

Name of the Instrument:

New Computerized Polygraph : Modular Model with Laptop and colour Printer- Qty.( 01)

(न्यू कम्प्यूटराईज्ड पालीग्राफ : माड्यूलर माडल विद लैपटॉप एण्ड कलर प्रिन्टर-1 अदद)

**Technical Specifications :**

1. Expandable upto 32 Channels with Laptop Computer and printer
2. Wired Modular Polygraph System
3. Preumo Module & Cardio Module
4. GSR/PLE Module includes EDA Cable, Metal Plates and 100 disposable electrodes.
5. Pump bulb
6. Arm cuff
7. PLE Finger Clip – Long
8. Activity Module includes : Seat Activity Sensor, Arms Feet
9. Docking station Holds Six Modules
10. Modular cable medium length- 36" UC shoulder Bag
11. Signature Pad Finger Print Reader
12. With seperately attached branded Web Cam of 5-8 mpxl.
13. With branded U.P.S.
14. USB to 18 PIN cable
15. Instrument should be quoted as a complete device at the time of installation.

Note: The instrument can be also purchased through STC process; New Delhi

**Accessories**

- Subject Chair

*S. Seth*  
4.2.15  
(Sangeeta Seth)  
S.O.  
F.S.L. U.P. LKO.

*Raj Kumar*  
4.2.15  
(Dr. Raj Kumar)  
D.D. Sero  
F.S.L. U.P. LKO.

*Suresh Chandra*  
4.2.15  
(Suresh Chandra)  
D.D. Bio  
F.S.L. U.P. LKO.

Lie Det. P

*S. Seth*  
प्रतिहस्ताक्षरित  
निदेशक  
विधि विज्ञान प्रयोगशाला  
उ० प्र०, लखनऊ

9125  
41872142-1  
TS-MOD-109/2015

## COMPARISON MICROSCOPE

### Specifications :-

#### A- Instrument part

Comparison Microscope should have basic stand with motorized height-adjustable column (Z range 250 mm or higher) including motorized comparison bridge with push button operation, integrated tiltable binocular head adjusting from 5- 35 degree. Field of view 22 mm; Upright & Non-reversed image, micro photo & video documentation port.

Motorized Comparison Bridge having following facilities

- Viewing of image 100% Right & 100% Left, both.
- Side-by-side image comparison with superimposed image.
- Adjustable and variable width of the dividing line.
- Motorized magnification changer with factor = 1x and 1.5x

Two macro carrier with macro tube lens, filter slots and coded 6-fold objective turret, two motorized X-Y stages (stage surface 150 x 120 mm or more with and travel range 50 x 50 mm or more), integrated operating panel for the control of the bridge functions, focusing, motorized X-Y movement of the stages, remote control of two cold light sources.

Motorized ergo-workbench with universal power supply and motorized height-adjustable work table with integrated toggle switch or optional foot pedal operation, suitable size table with height adjustment Z movement.

#### Illumination

Cold light illuminator with LCD display. Cold light source for halogen reflector lamp, electronic stabilization of lamp power, continuous intensity adjustment with remote control cable via front panel. Fiber-optics light guide, bifurcated, flexible & Cold Light Bar.

OR

Flexible LED spot light with bifurcated fiber optic light guide & spot lens

#### Different Stages

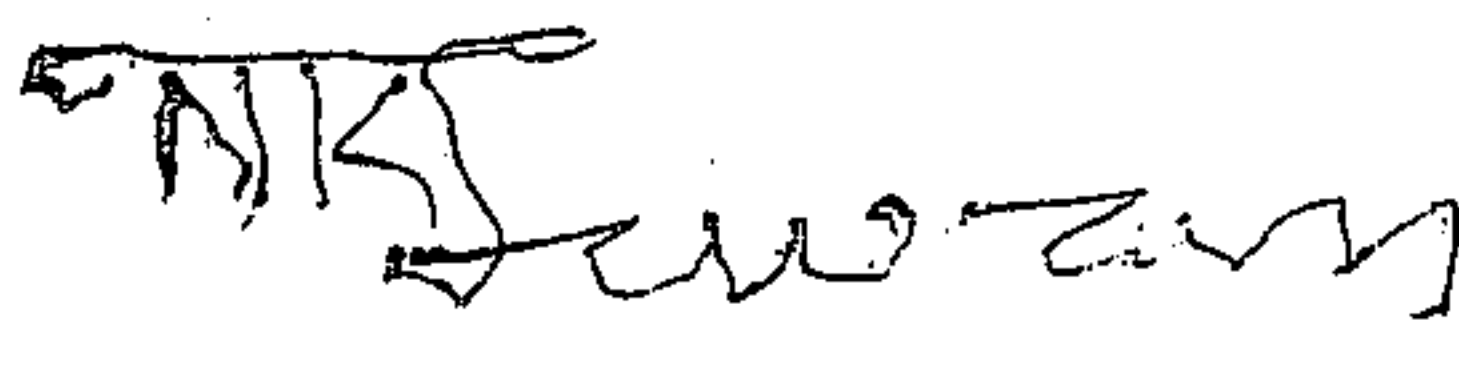
Rotating stage (110 mm dia. Or more) with stage rotation clamp, mountable on motorized stages.

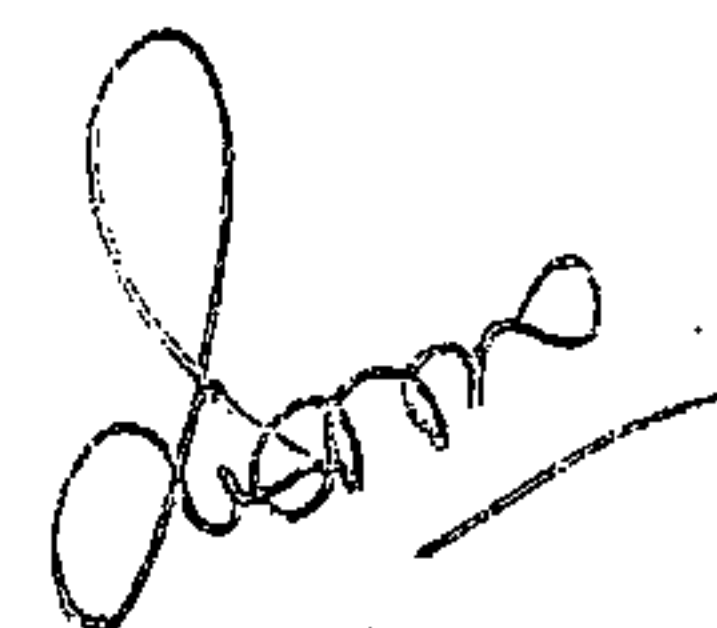
Attachable tilting stage (75 mm dia. Or more) and object clamp.

#### Optical Outfit

Apochromatic & HC (harmonic corrected) Macro-objectives: 0.4x, 1x, 2x, 4x with iris diaphragms and micro objectives, Eyepiece 10X/22 FOV. Magnification: 4x to 60x or more in the observation plane. All optics should be HC (Harmonic Component System) graded and

02  





62  
corrected. Supplementary lens 0.33x for 0.4x macro objective. Motorized condenser lens.

### **Different Specimen Holders**

Universal adjustable holder with rotating disc and accessories.

Set of calibration standards with grid structure.

Storage case for sample holders.

Articulated Arms with catch Device.

Pair of object stages diameter-60 mm with grooved profile and clamping device.

Pair of holder for lock cylinder.

Pair of wire holders for mounting cylindrical objects up to 7 mm diameter.

Pair of Rotatable Universal Shell holder.

Pair of Universal holders with rotating disc to mount various push in mounts, inclinable in segmental guides, scale divisions for reproducible rotation and inclination settings, dove tail guide for lateral displacement of segmental guides.

Pair of attachment for mounting and fixing bullets of various sizes.

Pair of Centering Device mounts for Bullets holder.

Pair of Cementing Stages dia. 20 mm for mounting bullets and objects of various sizes.

Pair of spring mounts for hunting cartridge cases.

Pair of attachable tilting stage diameter 25 mm with grooved profile and tilting fixture.

Pair of articulated holders with ball joints and tiring screws for tilting and rotating cartridge cases.

Pair of Push-in fixtures for deformed bullets.

Pair of mounts for air-gun ammunition.

Set of Brushes, Accessories plate.

### **Digital Imaging Workstation & Software**

Latest branded computer with color laser printer and UPS

C-mount adapter

### **Compatible High Resolution Digital FireWire Camera System**

For dedicated microscopy use

### **Suitable Image Processing & Analysis Software**

For Automatic measurement of multiple parameters

**Warranty** -Five (5) year on-site comprehensive warranty.

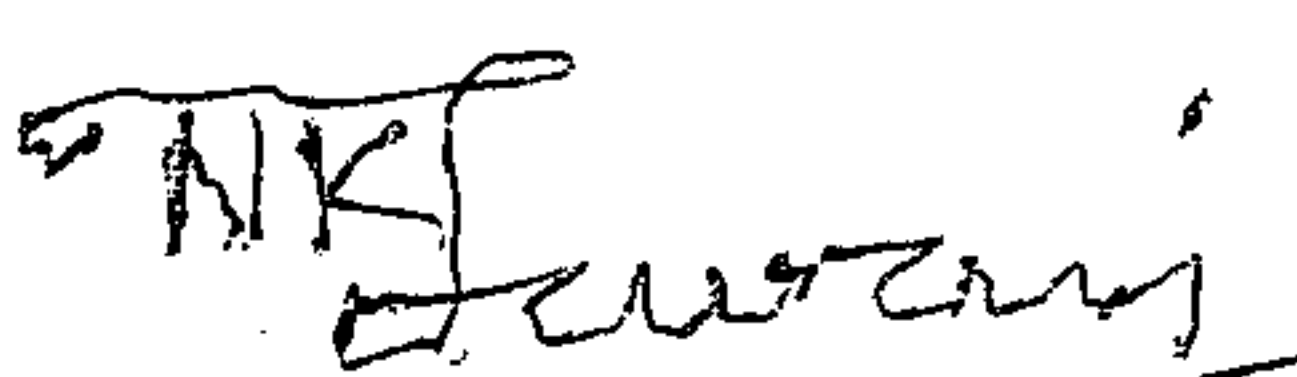
Quoted price must be in Indian Rupees.


61

Infrastructure part

- 1- Lab preparation – Size 15 x 15 feet with floor tile fixing, false ceiling, painting & wiring etc.
- 2- Split Air Conditioner (AC) – Two of 1.5 T capacity each.
- 3- Lab Work Station – Two of size 5 x 4 feet with chairs
- 4- Consumables & Chemicals etc.

  
Sanjay Khare  
SSA,

  
Dr. N. K. Tiwari  
Scientific Officer,  
FSL, Agra

  
Dr. Ram Janam  
Joint Director,  
FSL, Varanasi

TS-MOD-111/2015

Tender No. TS-MOD-111/2015-16/888

Name Of the Instrument: LAB COOLING DEVICE- FOR FORENSIC LAB: (AIR-CONDITIONING) Qty. (02)

**(Part-1) Proforma for Technical Specifications:-**

Main Features:-

(60) Testing rooms in Forensic Science Laboratory. UP. Mahanagar, Lucknow.

(A) Total Number of Testing/ Experimental Rooms/ Area: 60/2.0 Lacs Sq.ft. approx...

(B) Air Conditioning & Humidity Control Unit:-

To maintain the temperature, humidity, Clean Rooms; the all testing rooms should be covered with Clean room technology & Clean Air- ISO 14644-1 Clean room Standard's Class- 6; 1,00,000 maximum particles/m3 completely Dust-Free Bio- Hazardous, Echo-friendly & Energy- efficient good Environmental conditions required.

S N	Name & Items- Categories of Work	Technical Specifications	Quantity
1.	<b>Air Conditioning- Air Conditioning &amp; Humidity Control Unit:-</b> all the Forensic Divisions- (1) Receipt Division (2) Biology Division	(i) Air Conditioners & Humidity Control Unit should be of five (*) star rating & energy- efficient & turbo cooling. (ii) Dimensions of air cooling device (Minimum & Maximum standard Dimensions ) (iii) Standard make- model brand- Blue star, Carrier, Voltas, general, Lloyd & hitachi- Window/Split AC- Two (2 tone)/	30 AC

New Lab cooling device



	(3) Serology Division (4) Chemistry Division (5) Ballistics Division (6) Toxicology Division (7) Physics Division (8) Document Division (9) Photo Division (10) Instrument Division (11) Computer Division (12) Computer Forensic (13) Library (14) Museum (15) Front and back area	One & half (1.5 tone). (Depending upon the feasibility & area of testing rooms.) (iv) All parts of air conditioning unit should be of corrosion proof plastic, stainless-steel, galvanized steel, brass or copper make. (v) Instrument should be echo- friendly, CFC free & provided with anti- bacteria & active carbon free filtration with revolving grills minimum noise level. The air conditioners must be with anti corrosive blue- fine rotary type condenser with minimum five year warranty. The instrument should have in built facility of sleep mode & on-off time with elegant remote control of LCD with back light. All devices should be quoted as a complete device with branded suitable copper branded establishers. (vi) The instrument should be equipped with anti-freeze thermostat, auto defrosting system and wide range of air flow. (vii) The instrument should be quoted as a complete unit provided with suitable stabilizers at the time of installation.	
2	<b>Repairing of the Roof of FSL Building</b>	(i) Insulation and water proofing. (ii) The roof will be treated with standard (ISI) water proofing chemicals and creating sufficient slope for water draining. (iii) All roofs will be covered with standard jointless vitrified scratch resistant tiles (2.5 mm X 60 cmX60cm) fitted over	1880 Sq. mt. approx..


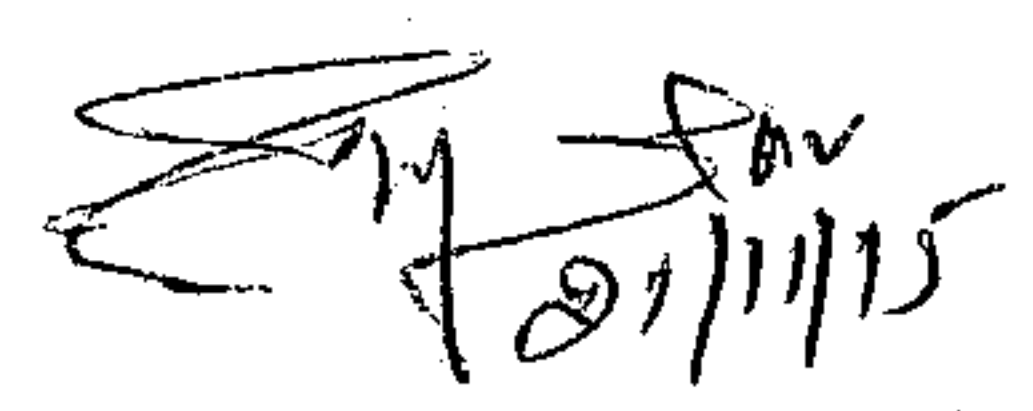


New Lab cooling device

21/11/15

21/11/15

		total roofs area. To ensure complete water proofing of roof. Heat resistant and exterior standard quality tiles.	
3.	<b>Electrical, Mechanical, Plumbing &amp; all type of Fabricating work</b>	(i) In all the testing rooms of both floors work of old doors, windows, ventilation and AC fitting should be finished with suitable aluminum gaze (35 mm width) and stainless steel.	No. of window.... etc. will be approx.. Nos. 48
4.	<b>Plastering of walls - of all divisions.</b>  <b>To make the lab dust and moisture free :-</b>	(i) Plastering of walls of all the divisions; Inner walls, Interior walls & Exterior walls of all the sections- rooms , Galleries, verandas, stairs and wash-rooms etc. using red coarse sand cement 6:1. The plaster should be even and no gap should be visible when aluminum leveler is placed on the walls. (ii) Plastering of walls work should be done on the basis of PWD norms with good quality cement and Morang ratio. (iii) Removal of old cements material from the walls in between the bricks up to the groove level.	Area 2.0 lac Sq feet approx..
5.	<b>White Cementing of all walls of all divisions+Putty for moist free environment:- Inner &amp; Outer portion</b>	(i) White Cementing of all the walls of all the division: Inner & Outer walls all the rooms. Size 100-500 micro meter moisture free, dust free for clean room maintenance Followed by even putty application the putty should be even out using sand paper if necessary. No striation should be visible. (ii) Including SCRB Wings.	All walls of mentioned area


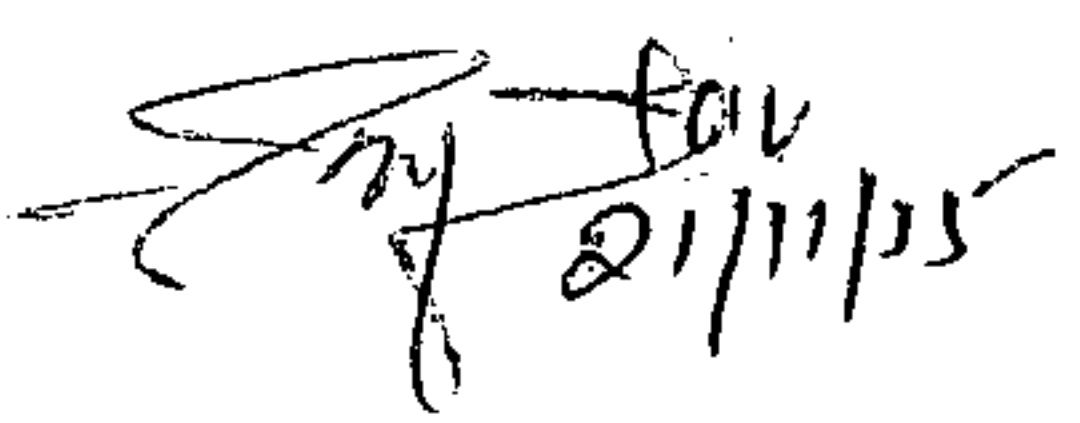

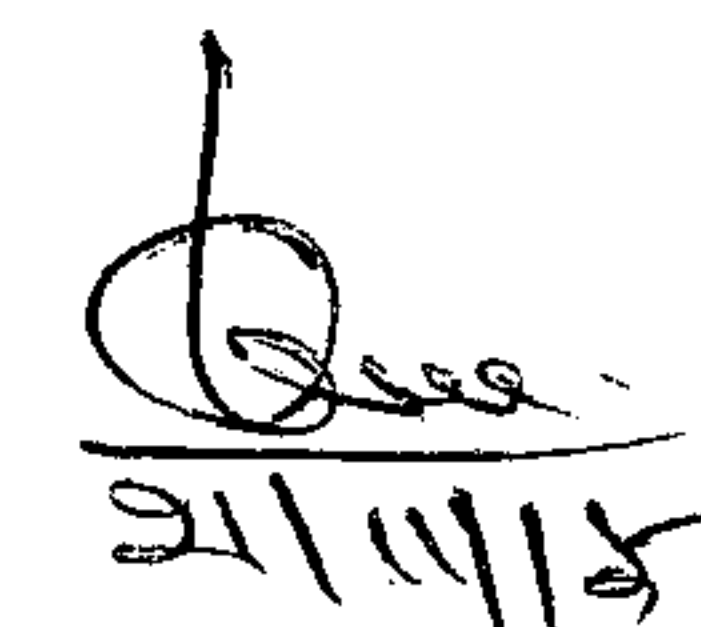
New Lab cooling device



6.	<b>Painting of all the walls of all divisions:- Inner &amp; Outer</b>	<p>Painting of all the walls of all the divisions- Inner &amp; Outer walls-.</p> <p>(i) All walls of testing rooms should be painted with two or more coats standard paints of (Burger/ Nerolac / Asian brand) paints.</p> <p>(ii) All walls should be properly sanded, preparing base with branded wall- putty for smoother &amp; proper finishing and application of primer.</p> <p>(iii) All testing rooms must be labeled with suitable name plates after completion of white wash- work.</p> <p>(iv) The painting should be washable, stain resistance, and remain spot less clean.</p> <p>(v) The painting should be done with anti- fungal shield Resistance to fungal growth.</p> <p>(vi) The painting of testing. rooms must be on basis of all surfaces enamel that forms a tough , washable , stain resistant film; The outer walls must be pointed whether points Imparting a new look to rooms, grills, gates &amp; window.</p>	All walls of mentioned area
7.	<b>Anti- termite &amp; Pest treatment of all the rooms, verandas, galleries, library &amp; museum on ground floor.</b>	<p>Anti - termite/ Pest control treatment should be done by drilling process covering all areas of wooden &amp; flooring places of testing rooms of ground floor.</p> <p>(i) The pesticides &amp; anti termite chemicals must be of standard quality.</p> <p>(ii) Quality; preferably- chloro pyriphos- oregano phosphorus.</p>	<b>Rooms, Verandas, Galleries, Library &amp; Museum on ground</b>

New Lab cooling device

		(ii) The treatment of anti termite & pesticides must be eco-friendly and non-hazardous. (iii) All mentioned area of testing rooms should be covered & treated with branded chemicals. (iv) All chemical should be for long lasting period.	<b>floor</b>
8.	<b>Flooring of all the rooms:-</b> of the both floors of the laboratory	Flooring of all the testing rooms should be furnished by: 600x600 mm vitrified scratch resistant tiles having 25 mm width. (i) Flooring tiles must be branded preferably - kajaria, Oasis, Jonson & Somani etc. quality. (ii) All works of flooring must be scratch furnished as a completed unit- including materials, fitting & labor charges etc. (iii) Flooring tiles must be made of more durable & eco-friendly material, with approved shades, ISO mark and nano technology grade. (iv) Flooring tiles must be according to the mentioned feature like- smoothness and shining with maximum resistance to the scratches and safer movement. (v) Flooring tiles must be easy to clean shine with low maintenance costs.	Area approx.. 37,000 sq feet
		<b>Total</b>	

New Lab cooling device

*[Signature]*

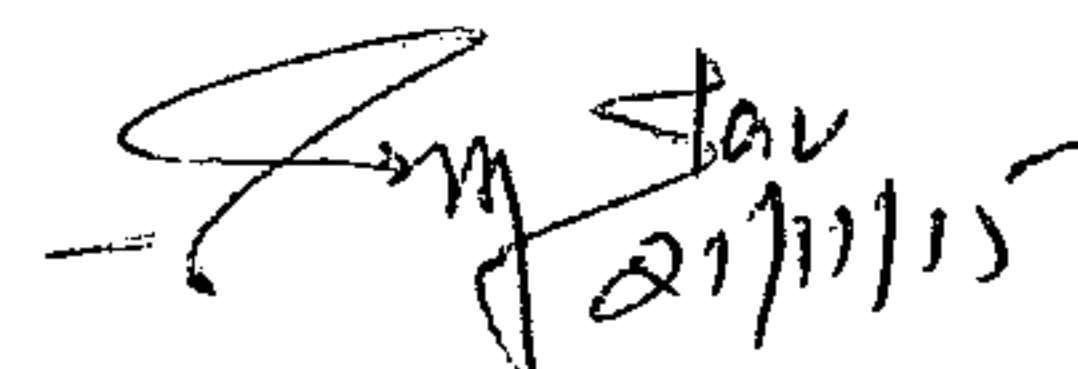
*[Signature]* 21/11/15


*[Signature]* 21/11/15

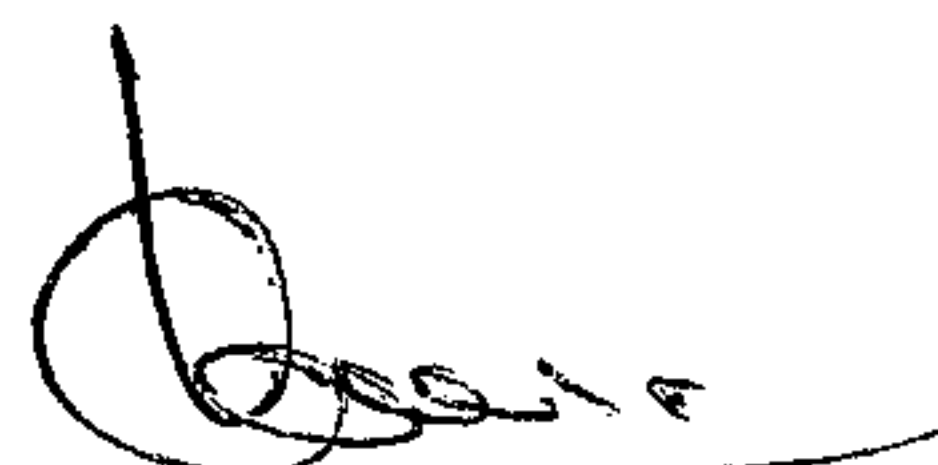
*[Signature]* 21/11/15

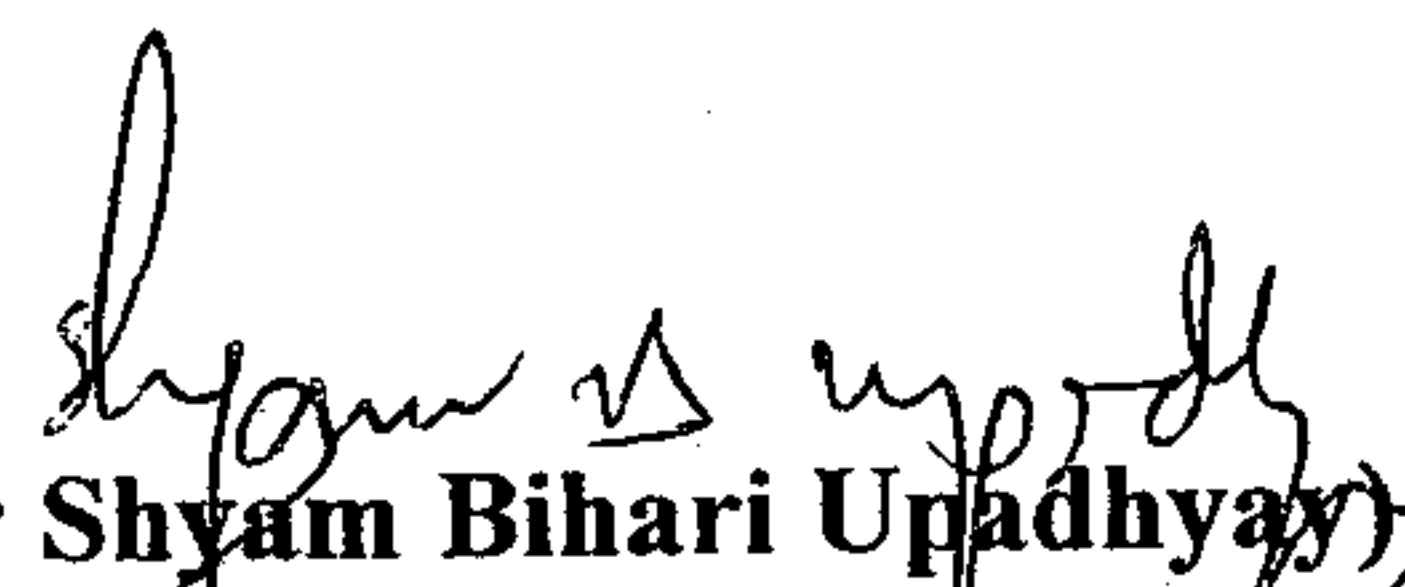


- (i) L1 will be decided based on total cast quoted including taxes.
- (ii) Calculation will be based on total area which is approximately given.
- (iii) However Payment will be made; based on actual work done.(running payment)
- (iv) Firm should coat rate of individual items unit wise.
- (v) Department reserves right to change or modify area of any item.
- (vi) In usual items as given above if firm completes 50 % of work, can claim part payment to the extent of work done.

  
( SN Yadav)  
Sr. Scientific Assisstant  
FSL UP Lucknow

  
(Dr Faizan Ahmad Khan)  
Scientific Officer  
FSL UP Lucknow

  
(Suresh Chandra)  
Deputy Director  
FSL UP Lucknow

  
(Dr Shyam Bihari Upadhyay)  
Director, FSL. UP.  
FSL UP Lucknow

New Lab cooling device

## Tender No. TS-MOD-109/2015-16/888

Name Of the Instrument: LAB COOLING DEVICE- FOR FORENSIC LAB: ( AIR-CONDITIONING ) Qty. (02)

### (Part-2 ) Proforma for Financial offer:-

Main Features:-

(60) Testing rooms in Forensic Science Laboratory. UP. Mahanagar, Lucknow.


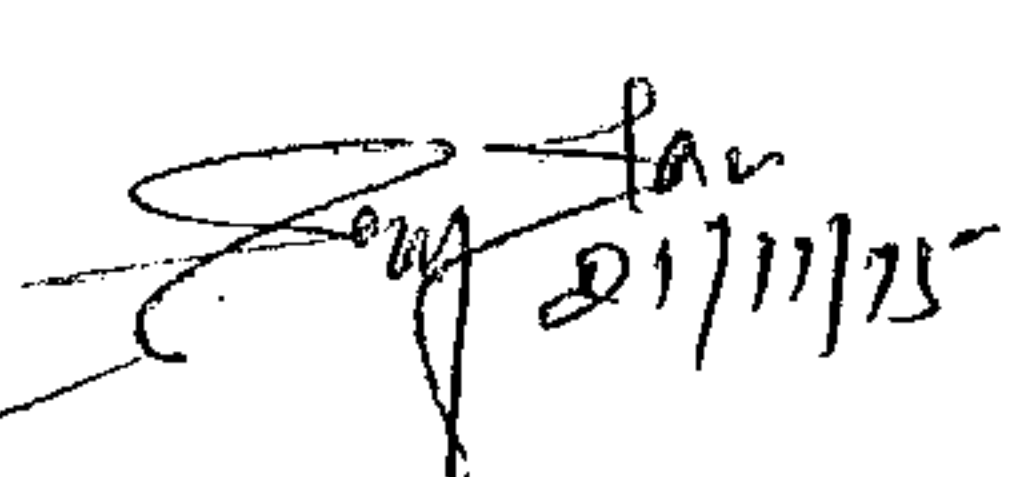

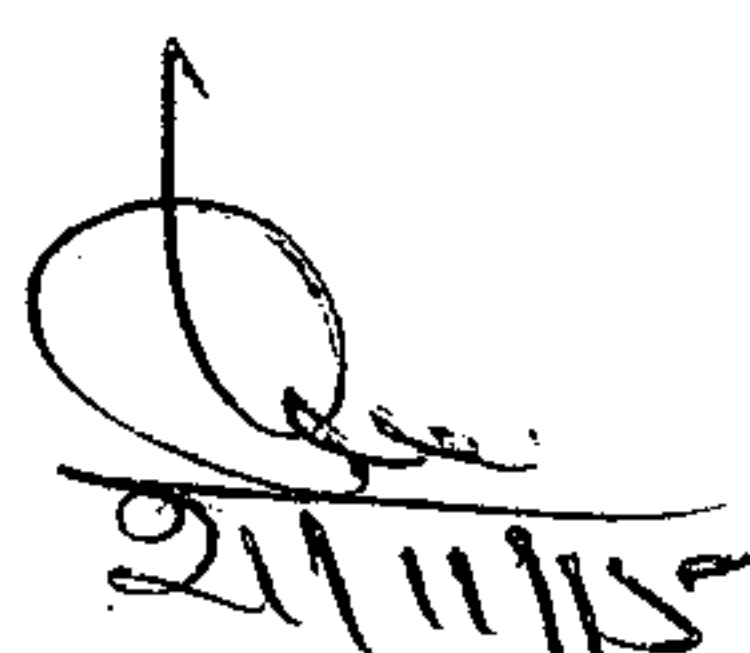
(A) Total Number of Testing/ Experimental Rooms/ Area: 60/2.0 Lacs Sq.ft.

(B) Air Conditioning & Humidity Control Unit:-

To maintain the temperature, humidity, Clean Rooms; the all testing rooms should be covered with Clean room technology & Clean Air- ISO 14644-1 Clean room Standard's Class- 6; 1,00,000 maximum particles/m3 completely Dust-Free Bio- Hazardous, Echo-friendly & Energy- efficient Good Environmental conditions required.

S N	Name & Items- Categories of Work	Technical Specifications	Quantity	Rate/ Unit	Total Amount
1.	<b>Air Conditioning- Air Conditioning &amp; Humidity Control Unit:-</b> all the Forensic Divisions- (1) Receipt Division (2) Biology Division	(i) Air Conditioners & Humidity Control Unit should be of five (*) star rating & energy- efficient & turbo cooling.  (ii) Dimensions of air cooling device (Minimum & Maximum standard Dimensions )	30 AC		


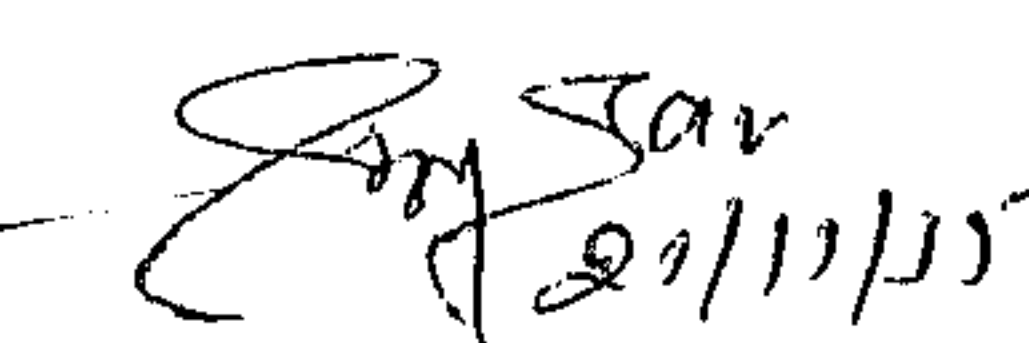

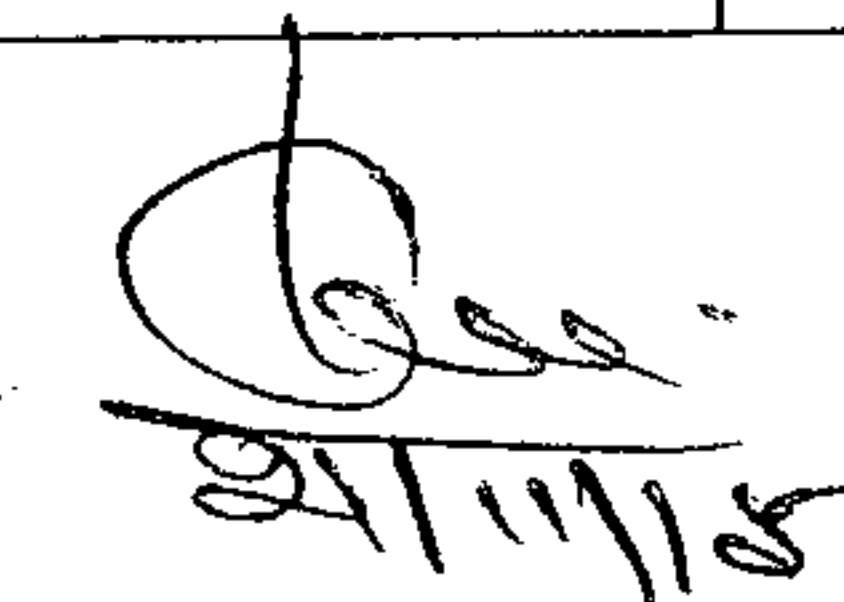
New Lab cooling device

  21/11/15  21/11/15  21/11/15




	(3) Serology Division (4) Chemistry Division (5) Ballistics Division (6) Toxicology Division (7) Physics Division (8) Document Division (9) Photo Division (10) Instrument Division (11) Computer Division (12) Computer Forensic (13) Library (14) Museum (15) Front and back area	(iii) Standard make- model brand- Blue star, Carrier, Voltas, general, Lloyd & hitachi- Window/Split AC- Two (2 tone)/ One & half (1.5 tone). (Depending upon the feasibility & area of testing rooms.) (iv) All parts of air conditioning unit should be of corrosion proof plastic, stainless-steel, galvanized steel, brass or copper make. (v) Instrument should be echo- friendly, CFC free & provided with anti- bacteria & active carbon free filtration with revolving grills minimum noise level. The air conditioners must be with anti corrosive blue- fine rotary type condenser with minimum five year warranty. The instrument should have in built facility of sleep mode & on- off time with elegant remote control of LCD with back light. All devices should be quoted as a complete device with branded suitable copper branded establishers. (vi) The instrument should be equipped with anti-freeze thermostat, auto defrosting system and wide range of air flow. (vii) The instrument should be quoted as a			
--	---	---	--	--	--

New Lab cooling device

		complete unit provided with suitable stabilizers at the time of installation.			
2	<b>Repairing of Roof of FSL Building</b>	(ii) Insulation and water proofing. (iii) The roof will be treated with standard (ISI) water proofing chemicals and creating sufficient slope for water draining. (iv) All roofs will be covered with standard jointless vitrified scratch resistant tiles (2.5 mm X 60 cmX60cm) fitted over total roofs area. To ensure complete water proofing of roof. Heat resistant and exterior standard quality tiles.	1880 Sq. mt. approx..		
3.	<b>Electrical, Mechanical, Plumbing &amp; all type of Fabricating work</b>	(i) In all the testing rooms of both floors work of old doors, windows, ventilation and AC fitting should be finished with suitable aluminum gaze (35 mm width) and stainless steel.	No. of window.... etc. will be approx.. Nos. 48		
4.	<b>Plastering of walls - of all divisions.</b>  <b>To make the lab dust and moisture free :-</b>	(i) Plastering of walls of all the divisions; Inner walls, Interior walls & Exterior walls of all the sections- rooms, Galleries, verandas, stairs and wash-rooms etc. using red coarse sand cement 6:1. The plaster should be even and no	Area 2.0 lac Sq feet approx..		

New Lab cooling device

 27/11/15

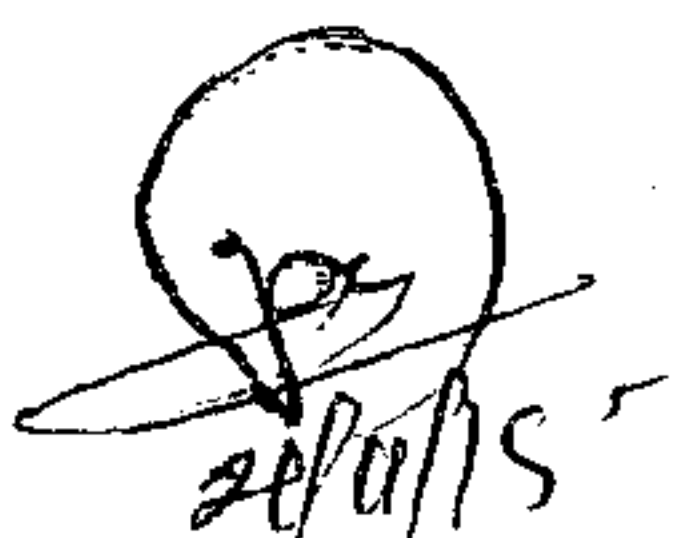
 27/11/15

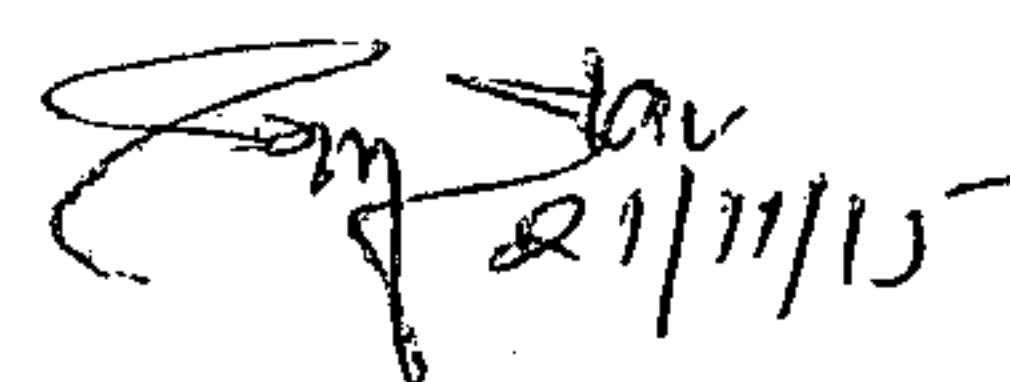
 27/11/15



		<p>gap should be visible when aluminum leveler is placed on the walls.</p> <p>(ii) Plastering of walls work should be done on the basis of PWD norms with good quality cement and Morang ratio.</p> <p>(ii) Removal of old cements material from the walls in between the bricks up to the groove level.</p>			
5.	<b>White Cementing of all walls of all divisions Putty</b> <b>For moist free environment:-</b> Inner & Outer portion	<p>(v) White Cementing of all the walls of all the division: Inner &amp; Outer walls all the rooms. Size 100-500 micro meter moisture free, dust free for clean room maintenance Followed by even putty application the putty should be even out using sand paper if necessary. No striation should be visible.</p> <p>(vi) Including SCRB Wings.</p>	All walls of mentioned area		
6.	<b>Painting of all the walls of all divisions:-</b> Inner & Outer	<p>Painting of all the walls of all the divisions- Inner &amp; Outer walls-.</p> <p>(i) All walls of testing rooms should be painted with two or more coats standard paints of (Burger/ Nerolac / Asian brand) paints.</p> <p>(ii) All walls should be properly sanded, preparing base with branded wall- putty for smoother &amp;</p>	All walls of mentioned area		

New Lab cooling device

  
20/11/15

  
21/11/15

  
21/11/15

		<p>proper finishing and application of primer.</p> <p>(iii) All testing rooms must be labeled with suitable name plates after completion of white wash-work.</p> <p>(iv) The painting should be washable, stain resistance, and remain spot less clean.</p> <p>(v) The painting should be done with anti- fungal shield Resistance to fungal growth.</p> <p>(vi) The painting of testing. rooms must be on basis of all surfaces enamel that forms a tough , washable , stain resistant film; The outer walls must be pointed whether points Imparting a new look to rooms, grills, gates &amp; window</p>			
7.	<b>Anti- termite &amp; Pest treatment of all the Rooms, Verandas, galleries, Library &amp; Museum on ground floor.</b>	<p>Anti - termite/ Pest control treatment should be done by drilling process covering all areas of wooden &amp; flooring places of testing rooms of ground floor.</p> <p>(i) The pesticides &amp; anti termite chemicals must be of standard quality.</p> <p>(ii) Quality; preferably- chloro pyriphos- oreghano phosphorus.</p> <p>(iii) The treatment of anti termite &amp; pesticides must be eco-friendly and non- hazardous.</p> <p>(iv) All mentioned area of testing rooms should be</p>	<b>Rooms, Verandas, Galleries, Library &amp; Museum on ground floor</b>		

New Lab cooling device

*[Signature]* 21/11/15


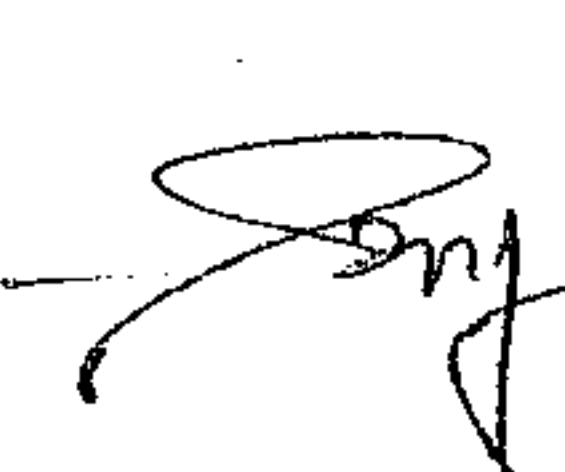
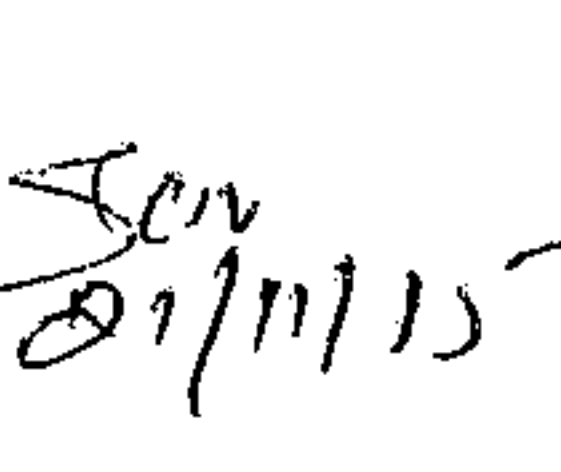

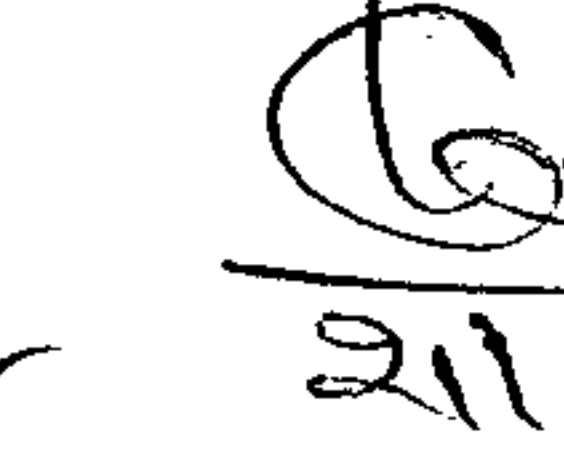
*[Signature]* 21/11/15

*[Signature]* 21/11/15

		covered & treated with branded chemicals. (v) All chemical should be for long lasting period.			
8.	<b>Flooring of all the rooms:-</b> of the both floors of the laboratory	<p>Flooring of all the testing rooms should be furnished by: 600x600 mm vitrified scratch resistant tiles having 25 mm width.</p> <p>(i) Flooring tiles must be scratch resistant branded preferably - kajaria, Oasis, Jonson &amp; Somani etc. quality.</p> <p>(ii) All works of flooring must be furnished as a completed unit- including materials, fitting &amp; labor charges etc.</p> <p>(iii) Flooring tiles must be made of more durable &amp; eco- friendly material, with approved shades, ISO mark and nano technology grade.</p> <p>(iv) Flooring tiles must be according to the mentioned feature like- smoothness and shining with maximum resistance to the scratches and safer movement.</p> <p>(v) Flooring tiles must be easy to clean shine with low maintenance costs.</p>	Area approx.. 37,000 sq feet		
		Total			

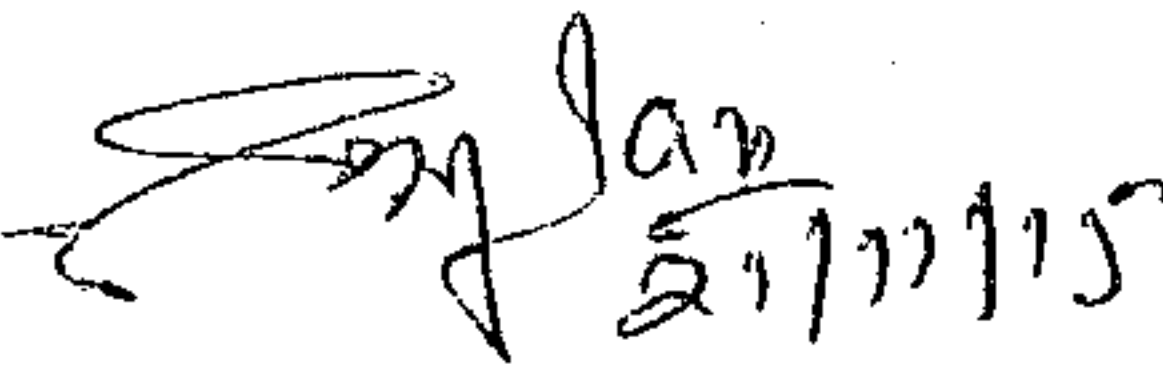
**Total Rs..... Taxes % Rs. .... Grand Total+ Taxes Rs.....**

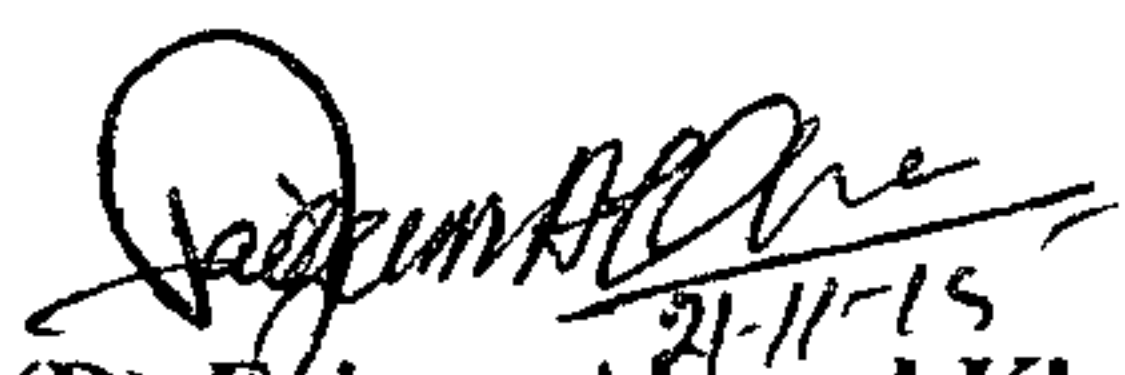
New Lab cooling device








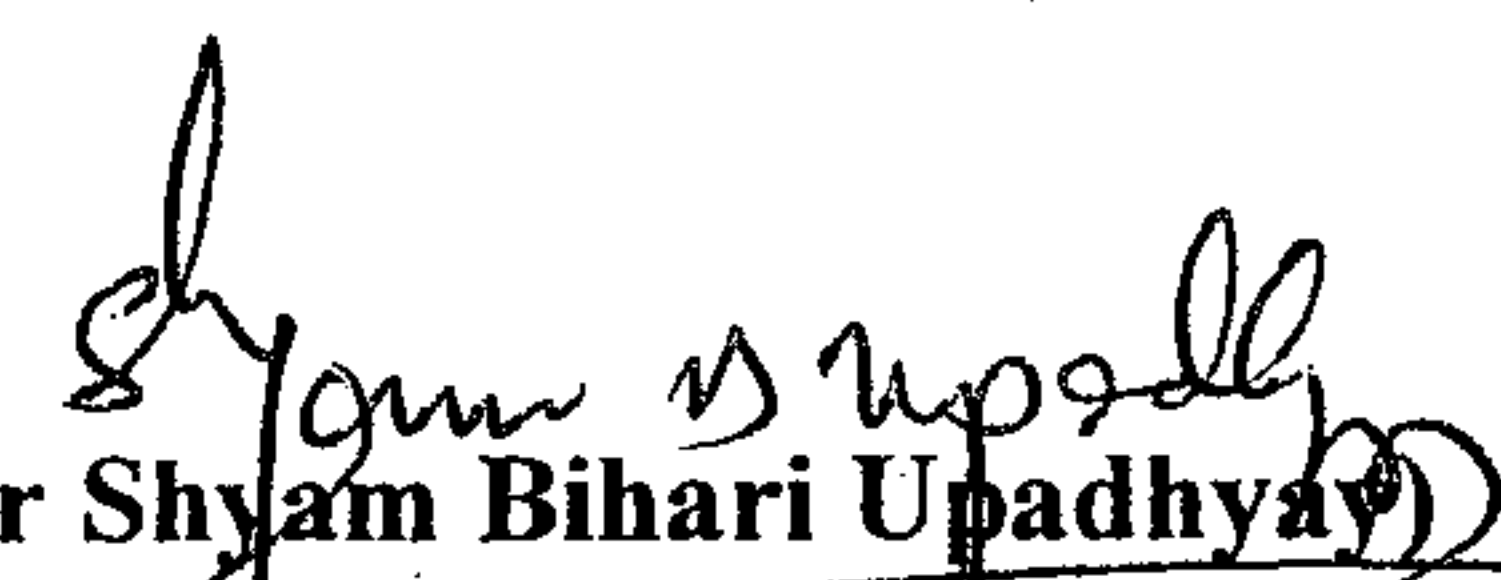


- (i) L1 will be decided based on total cast quoted including taxes.
- (ii) Calculation will be based on total area which is approximately given.
- (iii) However Payment will be made; based on actual work done.
- (iv) Firm should coat rate of individual items unit wise.
- (v) Department reserves right to change or modify area of any item.
- (vi) In usual items as given above if firm completes 50 % of work, can claim part payment to the extent of work done.

  
 (SN Yadav)  
 Sr. Scientific Assistant  
 FSL UP Lucknow

  
 (Dr Faizan Ahmad Khan)  
 Scientific Officer  
 FSL UP Lucknow

  
 (Suresh Chandra)  
 Deputy Director  
 FSL UP Lucknow  
 Dy: Director  
 Forensic Science Lab, U.P.  
 LUCKNOW-08

  
 (Dr Shyam Bihari Upadhyay)  
 Director, FSL. UP.  
 FSL UP Lucknow

New Lab cooling device

# TS-MOD - 135/2015-16

## SPECIFICATION OF LAB WORK STATION

### ISLAND BENCH:-L 3000mm x W 1500mm x H 900mm

- C Frame Structure in 32x32x1.2mm thick hollow Galvanized iron pipes with epoxy coating of high chemical resistance.
- Work top in  $18 \pm 1$  mm thick Jet Black Granite construction with moulding at the front and grooved at the bottom to protect module from chemicals.
- 750 mm wide storage module with two drawers and two shutters .
- 500 mm wide storage module with one drawer and one shutters
- 350 mm wide storage module with one drawer and one shutters
- Leg Space -2 Nos.(one side each).
- Doubled sided double tier reagent rack with electrical raceway.
- Electrical sockets 5/15 amp and switch/Tiny Trip – 12 Nos.
- Data Socket- 2 Nos (one side each).
- Single piece moulded PP Sink (L560xW355xD230)-1NO.
- Worktop mounted three way water tap with swan neck spout-1No.
- Peg Board in Phenolic Resin construction with 20 Nos PP Pegs -1No.
- Worktop mounted hand held type double outlet eye wash with SS breaded.
- Flexible hose -1No.
- Splash Guard.
- Sitting round stool with arm rest -4 Nos.

### WALL BENCH:-L 2450mm x W 750mm x H 900mm

- C Frame Structure in 32x32x1.2mm thick hollow Galvanized iron pipes with epoxy coated of high chemical resistance construction.
- Work top in  $18 \pm 1$  mm thick Black Granite construction.
- 750 mm wide storage module with one drawer and two shutters-1No.
- Worktop mounted electrical raceway.
- Electrical sockets 5/15 amp and switch/Tiny Trip – 8 Nos.
- Data Socket- 1 No.
- Leg Space – 1 No.(suitable to module dimension)
- Single piece moulded PP Sink (L560xW355xD230)-1NO. With mounted three way water tap with swan neck spout-1No.
- Flexible hose -1No.
- Sitting round stool with rest arm-2 Nos.

Please quote Island bench and wall bench separately with all necessary fittings and installation charges on site.

ZEBA KHAN  
SA

A K SINHA  
SO

Dr K K VERMA  
DD(CHEM)



## U.P. POLICE TECHNICAL SERVICES, HEAD QUARTERS,

IV<sup>th</sup> FLOOR, JAWAHAR BHAWAN, ASHOK MARG, LUCKNOW-226001

### GENERAL TERMS AND CONDITIONS FOR TENDERS

The details of specifications & instructions are to be followed strictly in accordance with the tender notice.

1 - The tendering firms are requested to submit the offer in TWO PARTS. The First Part will be named as Technical Offer & the Second Part will be called as Financial Offer. The technical offer as well as financial offer are to be prepared separately for each tender. BOTH TECHNICAL OFFER AND FINANCIAL OFFER PROPERLY SEALED IN SEPERATE COVERS, MUST BE KEPT IN ONE BIG ENVELOPE AND SEALED. ON EACH COVER INDICATE CLEARLY THE TENDER NO. \_\_\_\_\_ ITEM AND DATE \_\_\_\_\_ OPENING DUE ON \_\_\_\_\_. DO NOT QUOTE RATES IN THE TECHNICAL OFFER, OTHERWISE THE TENDER WILL BE REJECTED.

2- check list duly filled and signed with stamp must be submitted by the bidder.

2 - After submission of tender any addition, alteration or change in any offer shall not be acceptable.

3 - All the enclosures should be valid on the date of opening of the tender.

4 - If any cutting/ corrections, it should be properly attested by the tenderer.

5 - Earnest money (as mentioned in tender advertisement in news papers) has to be deposited FOR EACH ITEM SEPARATELY along with the Technical Offer in the form of Fixed Deposit of Scheduled Bank in the name of Superintendent of Police/ Asstt. Director, Uttar Pradesh Police Computer Center, payable at Lucknow,. Offers without earnest money will be ignored. If any firm is exempted from furnishing earnest money, enclose government orders. If government order is not submitted by the tenderer his tender will not be considered.

6 - It shall be the responsibility of the tendering firms to present themselves on the dates of opening of Technical & Financial offers and acquaint themselves with the short comings in the tender if any. No separate intimation will be sent to them in this regard.

7- Authorized Agent/ Dealer / Supplier/ Distributor should submit a self attested valid certificate of authority of their Principal/ Manufacturer. Manufacturer should attach a proof of which being so. Authorization is not necessary for Kits, Chemicals, Glassware, General Apparatus, Lab work station, furniture .

8 -Tenderer / Authorized person who shall sign the offer and all the enclosures submitted by them should have signature with their designation, seal and date.

9 - Quoted equipments should be complete working system with all necessary accessories including stabilizer / UPS, cables, wires etc. to run the system properly at the time of installation.

10 - Clearly mention installation requirements in the technical offer. Only space and electrical points will be provided at the time of installation. Installation of the supplied equipments shall be completed within 30 days from the date of receipt of equipment in this laboratory, failing which equipments costing up to Rs.5 lacks, penalty of Rs.100-00 per day and for every additional 5 lacks Rs.100-00 per day may be charged.

11- On Site Comprehensive Warranty of the equipments will be TWO YEARS on parts and labour or as specified below the specifications in the tender form from the date of supply and successful installation. Warranty of consumables and glass wares will be one year or as per their shelf life. Maintenance work of the supplied equipments shall be done by the supplier firm during warranty period.

12 - During warranty period, in case of local service centers complaints should be attended Next Business Day and in case of out station service centers complaints should be attended within 7 days, failing which equipments costing up to Rs.5 lacks penalty of Rs.100-00 per day and for every additional 5 lacks Rs.100-00 per day may be charged.



13 - Supply is to be executed as mentioned in the purchase order. Officer who is issuing purchase order can permit extra time on his discretion. If after making purchase agreement, any tenderer fails to supply goods of desired quality and quantity within 30 days in case of indigenous supply and 60 days in case of foreign supply, supply order may be cancelled and Security Money/Earnst money deposited by tenderer may be forfeited.

14 - Attach list of organizations to which the equipments have already been supplied and performance reports obtained from them with the technical offer.

15 -The items quoted should be of repute / standard brand. The tenderer should mention full particulars about the brand name, make, model, manufacturer and detailed specifications of the material offered by them with printed literature.

16 -Technical details as per tender specifications or their compatibility with the tender specifications shall be clearly mentioned in the technical offer.

17 - Firms shall quote in Indian Rupees and they must enclose (i) Self attested photocopy of valid U.P. Trade Tax Registration / Central Sales Tax / VAT Registration / latest Clearance Certificate (ii) photo copy of PAN / TAN no. (iii) Bank account no., name of bank and branch.

18 - The tenderer is required to submit an affidavit on 10 rupees stamp paper stating that :

(1)there is no dispute between the tenderer and state Govt./UP Police.

(2) the tenderer has no link with Mafia or some unsocial elements or organized crime.

19 - Quote rates including packing, forwarding, insurance, installation FOR destination any where in U.P. excluding all taxes and duties. However VAT, Entry Tax, other taxes and levies etc., should be mentioned separately. Rates should be quoted in two parts: 1- Cost of equipment with Two years on site comprehensive warranty, 2- Year wise charges for on site comprehensive annual maintenance contract from 3rd year to 5th year.

20 - After the receipt of goods in Forensic Science Laboratory, U.P., as specified in the purchase order( any district of U.P.), installation where needed shall have to be carried out by the firms at the required places within Uttar Pradesh.

21 - Any conditional discount on quantity basis (different discounts for different quantities) shall not be acceptable and such offers shall be rejected out rightly. However, unconditional discount given on quoted price on whole quantity, mentioned in financial offer only be acceptable.

22 - THE Technical Headquater RESERVES THE RIGHT TO ACCEPT OR REJECT ANY TENDER, EITHER IN PART OR FULL, WITHOUT ASSIGNING ANY REASON THERE OF.

23 - Firms must come prepared to demonstrate their goods in Forensic Science Laboratory, U.P., Mahanagar, Lucknow - 226006, on the next date of opening of technical bid. Demonstration will be asked if required, failing which tender will be rejected.

24 - The Technical Headquater has right to accept any lower or higher rates of the tenders without assigning any reason.

25- The validity of the rates should be at least for six months from the date of opening of the tender.

26 - In case of imported goods, foreign manufacturers can directly quote their rates but after sales service will be provided by their Indian Branch/ Agent. Name of trained engineers and details of service facilities available should be mentioned in technical offer.

27 - If Indian agents are quoting on behalf of foreign manufacturers/ Principals then self attested valid authority letter from them should be submitted along with the technical offer. Rates should be quoted in FOB as well as CIF Value at New Delhi air port.

28 - Tenderer have to accept one of the following payment terms:



OPTION-A: ON CAD TERMS i.e. 100% payment by Swift/ Wire Transfer to tenderer's Bank Account upon submission of required documents together with certificate of acceptance of equipment by the end-user's Department/Consignee to release 100% payment to the supplier.

OPTION-B: On LC Terms i.e. Letter of Credit for 100% value of the purchase order shall be established. Payment shall be released to the supplier by the Bank upon submission of documents to the bank by the beneficiary together with certificate of acceptance of equipment by the end-user's Department/Consignee after its installation. Bank charges in India shall be born by us whereas all bank charges in the foreign country, including confirmation charges of Letter of Credit, shall be to the account of the supplier.

29 - It will be the responsibility of the Indian agent of foreign principal to clear the consignment from customs and deliver it to Forensic Science laboratory, Lucknow/Agra/Varanasi as specified in the purchase order. The Indian Agent would bear the custom clearance charges (except custom duty), transportation charges, octroi etc. for supply of the goods to F.S.L. Lucknow/Agra/Varanasi.

30 - Forensic Science Laboratory, U.P., has to pay concessional customs duty. Custom duty at concessional rate certificate will be provided by FSL.

31 - Successful Tenderer will deposit 10% of the cost of equipment in India as security money and sign a purchase agreement within 7 days after receipt of purchase order on Rs. one hundred non judicial stamp paper at their own cost. Draft of purchase agreement shall be enclosed with the purchase order. Purchase order to the firms, who fail to execute the agreement shall be cancelled and EMD deposited by them shall be forfeited. Owner/partners of the firm /authorized person will sign purchase agreement. All signatures should be attested by notary. (authorized person will attach authority letter of owner / partners of the firm. )

32- Security Money will be in the form of Fixed Deposit of Scheduled Bank in the name of Superintendent of Police / Asstt. Director, Uttar Pradesh Police Computer Center, payable at Lucknow, or in the name of tenderer and pledged to Superintendent of Police / Asstt. Director, Uttar Pradesh Police Computer Center, Lucknow, which will be returned after expiry of warranty period.

33 - After thorough examination if the equipment delivered is found defective and unserviceable, it is to be replaced with new one within 30 days in case of indigenous items and 90 days in case of imported items. The expenditure incurred on this account will be borne by the "Supplier Firm". In case of inability to do so, the total cost of the equipment shall have to be refunded by the firm to the government of U.P.

34 - Bill to be submitted in triplicate by the firm in the name of Dy. Inspector General of Police, U.P. Police Technical Services, Head Quarters, Lucknow. Normally payment of bill will be made within 30 days but in case of delay no interest will be paid.

35 - Special Terms and conditions if any for any particular equipment has been mentioned below the specifications of the equipment in the tender form.

36 - If any item is on D.G.S & D/ D.I. rate contract enclose copy of rate contract along in the technical offer.

37 -Tendering firms will also impart hands on training for the supplied equipments wherever necessary free of cost.

38- Due to continuous research and developments and introduction of new models tendered can supply upgraded model at the same quoted price with permission of the department.

39 - Tendering firms should ensure that they will make available consumables, spares and services for equipments at least for ten years from the date of supply and installation.

40 - If supplier is unable to supply consumables, spares and services for ten years, he has to take back the supplied equipment and replace it by upgraded version free of cost.

41 - Supplier firm will provide driver software for new operating systems free of cost for ten years.

42 - Tenders received after the due date and time or incomplete tenders will not be accepted. This office will not be responsible for postal delay.

43 - Conditional tenders will not be accepted.

44 - If any firm will be defaulter of any terms and conditions given above the undersigned has right to deduct the part or full amount of the Earnest money/ Security money deposited by the firm, firm may be black listed and legal action may be taken.

45 - All disputes will be subject to jurisdiction of court at Lucknow only.

Following declaration form duly filled in and signed should be submitted along with the technical offer failing which tender will be rejected.

  
(Amitabh yash)  
Insp. Genl. Of Police, Technical Services,  
U.P. Police Technical Services, Lucknow

**DECLARATION**

I, (name of authorized representative)----- Son of-  
-----of M/S (Name of firm) -----  
-----have read all the rules of tender (1 to 45) given above. These are acceptable to  
our firm. Earnest Money in the form of Fixed Deposit of scheduled bank Rs.----- (in words)-----  
----- in favors of "Superintendent of Police / Asstt. Director, Uttar  
Pradesh Police Computer Centre, payable at Lucknow is enclosed herewith.

PLACE: -----

DATE-----

(Signature and seal)